



Enabling Legendary Discovery™

# **LEGENDplex™**

## Multi-Analyte Flow Assay Kit

### **Human Anti-Virus Response Panel Mix and Match Subpanel**

Please read the entire manual before running the assay.

BioLegend.com

***It is highly recommended that this manual be read in its entirety before using this product. Do not use this kit beyond the expiration date.***

*For Research Purposes Only. Not for use in diagnostic or therapeutic procedures. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of BioLegend is strictly prohibited.*

<b>Table of Contents</b>	<b>Page</b>
<b>Chapter 1: KIT DESCRIPTION</b> .....	3
Introduction.....	3
Principle of the Assay.....	3
Beads Usage.....	4
Storage Information.....	6
Materials Supplied.....	6
Materials to be Provided by the End-User.....	8
Precautions.....	9
<b>Chapter 2: ASSAY PREPARATION</b> .....	10
Sample Collection and Handling.....	10
Reagent Preparation... ..	10
Standard Preparation.....	11
Sample Dilution.....	12
<b>Chapter 3: ASSAY PROCEDURE</b> .....	13
Performing the Assay Using a Filter Plate.....	13
Performing the Assay Using a V-bottom Plate.....	16
<b>Chapter 4: FLOW CYTOMETER SETUP</b> .....	19
<b>Chapter 5: DATA ACQUISITION AND ANALYSIS</b> .....	19
Data Acquisition.....	19
Data Analysis.....	20
<b>Chapter 6: ASSAY CHARACTERIZATION</b> .....	21
Standard Curve.....	21
Assay Sensitivity.....	21
Cross-Reactivity.....	22
Accuracy.....	22
Linearity of Dilution.....	23

Human Anti-Virus Response Panel Mix and Match Subpanel

Intra-Assay Precision..... 24

Inter-Assay Precision..... 25

Biological Samples..... 26

**TROUBLESHOOTING**..... 29

**PLATE MAP**..... 33

## Chapter 1: KIT DESCRIPTION

### Introduction

In response to pathogens, especially viruses, cells release interferons and other cytokines to fight the infections. Interferons are typically divided into three types: 1 (e.g., INF- $\alpha$ , IFN- $\beta$ ), 2 (e.g., IFN- $\gamma$ ), and 3 (e.g., IFN- $\lambda$ 1, IFN- $\lambda$ 2). All interferons are important for fighting viral infections and for regulating the immune system. In addition, interferons are critically involved in cancer and autoimmune diseases such as psoriasis, systemic lupus erythematosus, and multiple sclerosis. Studying the expression profile of interferons and other related cytokines is pivotal to understand the immune responses against pathogens and related disease processes.

The LEGENDplex™ Human Anti-Virus Response Panel is a bead-based multiplex assay, utilizing fluorescence–encoded beads suitable for use on various flow cytometers. This panel allows simultaneous quantification of 13 human proteins, including interferons ( $\alpha$ ,  $\beta$ ,  $\gamma$ ,  $\lambda$ 1 and  $\lambda$ 2/3), interleukins (1 $\beta$ , 6, 8, 10, 12), TNF- $\alpha$ , IP-10 and GM-CSF. The Type 1/2/3 Interferon Panel is a subpanel of the 13-plex Anti-Virus Response Panel, which allows for simultaneous quantification of the five Interferons. Both panels provide high sensitivities and broad dynamic range. The two panels have been validated for use on serum and cell culture supernatant samples. Use plasma samples with caution due to sample viscosity and existence of particulates in such samples.

The Anti-Virus Response Panel is designed to allow flexible customization within the panel. Please visit [www.biolegend.com/legendplex](http://www.biolegend.com/legendplex) for more information on how to mix and match within the panel.

This assay is for research use only.

### Principle of the Assay

BioLegend's LEGENDplex™ assays are bead-based immunoassays using the same basic principle as sandwich immunoassays.

Beads are differentiated by size and internal fluorescence intensities. Each bead set is conjugated with a specific antibody on its surface and serves as the capture beads for that particular analyte. When a selected panel of capture beads is mixed and incubated with a sample containing target analytes specific to the capture antibodies, each analyte will bind to its specific capture beads. After washing, a biotinylated detection antibody cocktail is added, and each detection antibody in the cocktail will bind to its specific analyte bound on the capture beads, thus forming capture bead-analyte-detection antibody sandwiches. Streptavidin-phycoerythrin (SA-PE) is subsequently added, which will bind to the biotinylated detection antibodies, providing fluorescent signal intensities in proportion to the amount of bound analytes.

# Human Anti-Virus Response Panel Mix and Match Subpanel


Since the beads are differentiated by size and internal fluorescence intensity on a flow cytometer, analyte-specific populations can be segregated and PE fluorescent signal quantified. The concentration of a particular analyte is determined using a standard curve generated in the same assay.

## Beads Usage

The Anti-Virus Response Panel uses two sets of beads. Each set has a unique size that can be identified based on their forward scatter (FSC) and side scatter (SSC) profiles (Beads A and Beads B, Figure 1). Each bead set can be further resolved based on their internal fluorescence intensities. The internal dye can be detected using FL3, FL4, or APC channel, depending on the type of flow cytometer used. The smaller Beads A consists of 6 bead populations and the larger Beads B consists of 7 bead populations (Figure 2-3).

Using a total of 13 bead populations distinguished by size and internal fluorescent dye, the Anti-Virus Response Panel allows simultaneous detection of 13 proteins in a single sample. Each analyte is associated with a particular bead set as indicated (Figures 2-3 and Table 1).


**Figure 1. Beads Differentiated by Size**

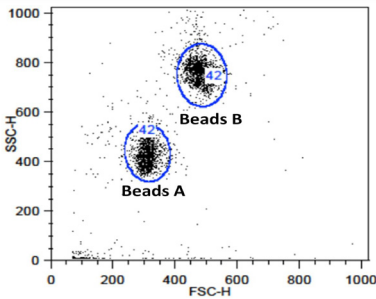

Beads A = smaller beads


Beads B = larger beads

**Figure 2. Beads A Classification by FL4**

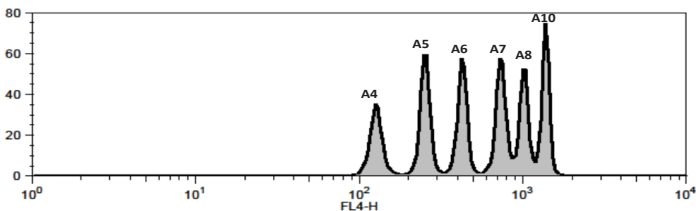

# Human Anti-Virus Response Panel Mix and Match Subpanel

**Figure 3. Beads B Classification by FL4**

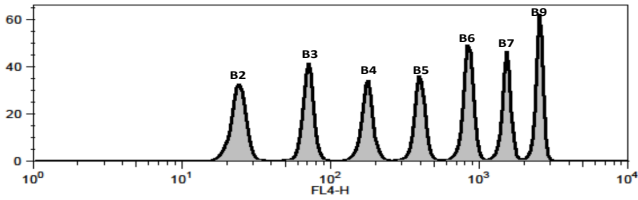

For Beads usage in various panels, please refer to Table 1 below:

**Table 1. Beads ID, Panel Specific Target Selection and Target information**

Target	Bead ID	Full Panel Cat# 740349* &740390**	Sunpanel Cat# 740350* &740396**	Top Standard Concentrations (ng/mL)
IL-1 $\beta$	A4	√		Note: The top standard concentrations of analytes in this panel were set at various concentrations, but may be subject to change from lot to lot (please visit <a href="http://biolegend.com/en-us/legendplex">biolegend.com/en-us/legendplex</a> to download a lot-specific certificate of analysis).
IL-6	A5	√		
TNF- $\alpha$	A6	√		
IP-10	A7	√		
IFN- $\lambda$ 1 (IL-29)	A8	√	√	
IL-8	A10	√		
IL-12p70	B2	√		
IFN- $\alpha$ 2	B3	√	√	
IFN- $\lambda$ 2/3 (IL-28A/B)	B4	√	√	
GM-CSF	B5	√		
IFN- $\beta$	B6	√	√	
IL-10	B7	√		
IFN- $\gamma$	B9	√	√	

**\* Cat# for kit with Filter plate. \*\*Cat# for kit with V-bottom Plate**

Bead ID is used to associate a bead population to a particular analyte when using the LEGENDplex™ data analysis software program. For further information regarding the use of the program please visit [biolegend.com/en-us/legendplex](http://biolegend.com/en-us/legendplex).

# Human Anti-Virus Response Panel Mix and Match Subpanel

## Storage Information

Recommended storage for all original kit components is between 2°C and 8°C. DO NOT FREEZE Beads, Detection Antibodies or SA-PE.

- Once the standards have been reconstituted, immediately transfer contents into polypropylene vials. DO NOT STORE RECONSTITUTED STANDARDS IN GLASS VIALS.
- Upon reconstitution, leftover standard and Matrix B should be stored at ≤-70°C for use within one month. Avoid multiple (>2) freeze-thaw cycles. Discard any leftover diluted standards.

## Materials Supplied

The LEGENDplex™ kit contains reagents for 100 tests, listed in the table below. When assayed in duplicate, this is enough for an 8-point standard curve and 40 samples.

For the Mix and Match Subpanels, individual beads are provided at 13X concentration. The Buffer Set contains Setup Beads, all Buffers, Plate Sealers, Matrix, and SA-PE.

Kit Components	Quantity	Volume	Cat #
<b>Capture Beads* (see tables below for more information)</b>	<b>varies</b>	270 µL	<b>varies</b>
LEGENDplex™ Human Anti-Virus Response Panel Detection Antibodies	1 bottle	3.5 mL	740364
LEGENDplex™ Human Anti-Virus Response Panel Standard	1 vial	lyophilized	740365
LEGENDplex™ Buffer Set A	1		740368
Filter Plate* or V-bottom Plate**	1 Plate		740377* or 740379**

\* For kit with filter plate. \*\* For kit with V-bottom plate.



## Human Anti-Virus Response Panel Mix and Match Subpanel

### Capture beads for Mix and Match Subpanels:

Bead Name	Quantity	Volume	Cat#
LEGENDplex™ Human IFN- $\alpha$ 2 Capture Bead B3, 13X	1 vial	270 $\mu$ L	740351
LEGENDplex™ Human IFN- $\gamma$ Capture Bead B9, 13X	1 vial	270 $\mu$ L	740352
LEGENDplex™ Human IFN- $\beta$ Capture Bead B6, 13X	1 vial	270 $\mu$ L	740353
LEGENDplex™ Human IFN- $\lambda$ 1 Capture Bead A8, 13X	1 vial	270 $\mu$ L	740354
LEGENDplex™ Human IFN- $\lambda$ 2/3 Capture Bead B4, 13X	1 vial	270 $\mu$ L	740355
LEGENDplex™ Human IL-6 Capture Bead A5, 13X	1 vial	270 $\mu$ L	740356
LEGENDplex™ Human IL-8 Capture Bead A10, 13X	1 vial	270 $\mu$ L	740357
LEGENDplex™ Human IL-10 Capture Bead B7, 13X	1 vial	270 $\mu$ L	740358
LEGENDplex™ Human TNF- $\alpha$ Capture Bead A6, 13X	1 vial	270 $\mu$ L	740359
LEGENDplex™ Human IL-12p70 Capture Bead B2, 13X	1 vial	270 $\mu$ L	740361
LEGENDplex™ Human GM-CSF Capture Bead B5, 13X	1 vial	270 $\mu$ L	740362
LEGENDplex™ Human IP-10 Capture Bead A7, 13X	1 vial	270 $\mu$ L	740363
LEGENDplex™ Human IL-1 $\beta$ Capture Bead A4, 13X	1 vial	270 $\mu$ L	740119

Please refer to Beads ID and Panel-Specific Target Selection table (Table 1), to see which capture beads are included in each panel.

### LEGENDplex™ Buffer Set A (Cat#: 740368)

Component	Quantity	Volume	Part #
Setup Beads 1: FITC Beads	1 vial	1 mL	77840
Setup Beads 2: PE Beads	1 vial	1 mL	77842
Setup Beads 3: Raw Beads	1 vial	2 mL	77844
LEGENDplex™ SA-PE	1 bottle	3.5 mL	77743
LEGENDplex™ Matrix B, Lyophilized	1 vial	lyophilized	77549
LEGENDplex™ Assay Buffer	1 bottle	25 mL	77562
LEGENDplex™ Wash Buffer, 20X	1 bottle	25 mL	77564
Plate Sealers	4 sheets		78101

No plate is included in Buffer Set A. Plate need to be ordered separately.

Please order the correct type of plate based on the preferred assay protocol (Cat# 740377 for Filter Plate and Cat# 740379 for V-bottom Plate)

# Human Anti-Virus Response Panel Mix and Match Subpanel

## Materials to be Provided by the End-User

- A flow cytometer equipped with two lasers (e.g., a 488 nm blue laser or 532 nm green laser and a 633-635 nm red laser) capable of distinguishing 575 nm and 660 nm or a flow cytometer equipped with one laser (e.g., 488 nm blue laser) capable of distinguishing 575 nm and 670 nm.

### Partial list of compatible flow cytometers:

Flow Cytometer	Reporter Channel	Channel Emission	Classification Channel	Channel Emission	Compensation needed?
BD FACSCalibur™ (single laser)	FL2	575 nm	FL3	670 nm	Yes
BD FACSCalibur™ (dual laser)	FL2	575 nm	FL4	660 nm	No*
BD FACSAria™	Yellow	575 nm	Red	660 nm	No*
BD FACSCanto™ BD FACSCanto™ II	PE	575 nm	APC	660 nm	No*
BD™ LSR, LSR II BD LSRFortessa™	PE	575-585 nm	APC	660 nm	No*
BD FACSAria™	PE	575 nm	APC	660 nm	No*

**\*Compensation is not required for the specified flow cytometers when set up properly, but is recommended for consistent results.**

For setting up of the above flow cytometers, please follow the **Flow Cytometer Setup** guide in this manual or visit: [www.biolegend.com/legendplex](http://www.biolegend.com/legendplex).

For flow cytometers not listed here, the end-user needs to set up the machine following similar guidelines. Please refer to **Setup Procedure for Other Flow Cytometers** section in Chapter 4.

- Multichannel pipettes capable of dispensing 5 µL to 200 µL
- Reagent reservoirs for multichannel pipette
- Polypropylene microcentrifuge tubes (1.5 mL)
- Laboratory vortex mixer
- Sonicator bath (e.g., Branson Ultrasonic Cleaner model #B200, or equivalent)
- Aluminum foil
- Absorbent pads or paper towels
- Plate shaker (e.g., Lab-Line Instruments model #4625, or equivalent)
- Tabletop centrifuges (e.g., Eppendorf centrifuge 5415 C, or equivalent)

## Human Anti-Virus Response Panel Mix and Match Subpanel

- 1.1 mL polypropylene micro FACS tubes, in 96-tube rack (e.g., National Scientific Supply Co, cat # TN0946-01R, or equivalent)

### **If the assay is performed in a filter plate,**

- A vacuum filtration unit (Millipore MultiScreen<sup>®</sup> HTS Vacuum Manifold, cat # MSVMHTS00 or equivalent). Instructions on how to use the vacuum manifold can be found at the supplier's website.
- A vacuum source (mini vacuum pump or line vacuum, e.g., Millipore Vacuum Pump, catalog # WP6111560, or equivalent).
- If needed, additional Filter plate can be ordered from BioLegend (Cat# 740377 or 740378).

### **If the assay is performed in a V-bottom plate,**

- Centrifuge with a swinging bucket adaptor for microtiter plates (e.g., Beckman Coulter Allegra™ 6R Centrifuge with MICROPLUS CARRIER adaptor for GH3.8 and JS4.3 Rotors).
- If needed, additional V-bottom plate can be ordered from BioLegend (Cat# 740379).

## **Precautions**

- All blood components and biological materials should be handled as potentially hazardous. Follow universal precautions as established by the Center for Disease Control and Prevention and by the Occupational Safety and Health Administration when handling and disposing of infectious agents.
- Sodium azide has been added to some reagents as a preservative. Although the concentrations are low, sodium azide may react with lead and copper plumbing to form highly explosive metal azides. On disposal, flush with a large volume of water to prevent azide build-up.
- Matrix B for LEGENDplex™ kits contains components of human origin and should be handled as potentially hazardous. The raw material has been screened for infectious diseases and is negative for HIV, HBV and HCV using FDA-approved test methods.
- Do not mix or substitute reagents from different kits or lots. Reagents from different manufacturers should not be used with this kit.
- Do not use this kit beyond its expiration date.
- SA-PE and Beads are light-sensitive. Minimize light exposure.

## Chapter 2: ASSAY PREPARATION

### Sample Collection and Handling

#### Preparation of Serum Samples:

- Allow the blood to clot for at least 30 minutes and centrifuge for 10 minutes at 1,000 x *g*.
- Remove serum and assay immediately or aliquot and store samples at  $\leq -20^{\circ}\text{C}$ . Avoid multiple (>2) freeze/thaw cycles.
- When using frozen samples, it is recommended that samples are thawed completely, mixed and centrifuged to remove particulates prior to use.

#### Preparation of Plasma Samples:

- Plasma collection using EDTA as an anti-coagulant is recommended. Centrifuge for 10 minutes at 1,000 x *g* within 30 minutes of blood collection.
- Remove plasma and assay immediately, or aliquot and store samples at  $\leq -20^{\circ}\text{C}$ . Avoid multiple (>2) freeze/thaw cycles.
- When using frozen samples, it is recommended that samples are thawed completely, mixed well and centrifuged to remove particulates.

#### Preparation of Tissue Culture Supernatant:

- Centrifuge the sample to remove debris and assay immediately. If not possible, aliquot and store samples at  $\leq -20^{\circ}\text{C}$ . Avoid multiple (>2) freeze/thaw cycles.

### Reagent Preparation

#### Preparation of Antibody-Immobilized Beads

The individual beads (13X) should be mixed and diluted to 1X with Assay Buffer prior to use. To mix the beads, follow the steps below (a 5-plex subpanel is used as an example):

1. Sonicate the beads vials for 1 minute in a sonicator bath and then vortex for 30 seconds prior to use.
2. Calculate the amount of mixed and diluted beads needed for the assay. Prepare extra to compensate for pipetting loss. Each reaction needs 25  $\mu\text{L}$  of mixed and diluted beads. For 50 reactions, prepare 1.5 mL of mixed beads. For 96 reactions, prepare 3 mL of mixed beads.

## Human Anti-Virus Response Panel Mix and Match Subpanel

3. To make 1.5 ml of 5-plex 1X diluted beads, transfer 115  $\mu\text{L}$  of each of the 5 individual beads (13X) to a fresh tube (total bead volume = 575  $\mu\text{L}$ ) and add 925  $\mu\text{L}$  of Assay Buffer to make the final volume of 1.5 mL.

### Preparation of Wash Buffer

- Bring the 20X Wash Buffer to room temperature and mix to bring all salts into solution.
- Dilute 25 mL of 20X Wash Buffer with 475 mL deionized water. Store unused portions between 2°C and 8°C for up to one month.

### Preparation of Matrix B (for Serum or Plasma Samples Only)

- Add 5.0 mL LEGENDplex™ Assay Buffer to the bottle containing lyophilized Matrix B. Allow at least 15 minutes for complete reconstitution. Vortex to mix well. Leftover reconstituted Matrix B should be stored at  $\leq -70^\circ\text{C}$  for up to one month.

### Standard Preparation

1. Prior to use, reconstitute the lyophilized Human Anti-Virus Response Panel Standard with 250  $\mu\text{L}$  Assay Buffer.
2. Mix and allow the vial to sit at room temperature for 10 minutes, and then transfer the standard to an appropriately labeled polypropylene microcentrifuge tube. This will be used as the top standard C7.

**Note: The top standard concentrations of analytes in this panel were set at various concentrations, but may be subject to change from lot to lot (please visit [biolegend.com/en-us/legendplex](http://biolegend.com/en-us/legendplex) to download a lot-specific certificate of analysis).**

3. Label 6 polypropylene microcentrifuge tubes as C6, C5, C4, C3, C2 and C1, respectively.
4. Add 75  $\mu\text{L}$  of Assay Buffer to each of the six tubes. Prepare 1:4 dilution of the top standard by transferring 25  $\mu\text{L}$  of the top standard C7 to the C6 tube and mix well. This will be the C6 standard.
5. In the same manner, perform serial 1:4 dilutions to obtain C5, C4, C3, C2 and C1 standards (**see the table below using the top standard at 10,000 pg/mL as an example**). Assay Buffer will be used as the 0 pg/mL standard (C0).

## Human Anti-Virus Response Panel Mix and Match Subpanel

Tube/ Standard ID	Serial Dilution	Assay Buffer to add ( $\mu$ L)	Standard to add	Final Conc. ( $\mu$ g/mL)*
C7	--	--	--	10,000
C6	1:4	75	25 $\mu$ L of C7	2,500
C5	1:16	75	25 $\mu$ L of C6	625
C4	1:64	75	25 $\mu$ L of C5	156.3
C3	1:256	75	25 $\mu$ L of C4	39.1
C2	1:1024	75	25 $\mu$ L of C3	9.8
C1	1:4096	75	25 $\mu$ L of C2	2.4
C0	--	75	--	0

### Sample Dilution

- Serum or plasma samples must be diluted 2-fold with Assay Buffer before being tested (e.g. dilute 50  $\mu$ L of sample with 50  $\mu$ L of Assay Buffer).

If further sample dilution is desired, dilution should be done with Matrix B to ensure accurate measurement.

**Adding serum or plasma samples without dilution will result in low assay accuracy and possibly, clogging of the filter plate.**

- For cell culture supernatant samples, the levels of analyte can vary greatly from sample to sample. While the samples can be tested without dilutions, a preliminary experiment may be required to determine the appropriate dilution factor.

If sample dilution is desired, dilution should be done with corresponding fresh cell culture medium or Assay Buffer to ensure accurate measurement.

## Chapter 3: ASSAY PROCEDURE

The LEGENDplex™ assay can be performed in a filter plate, or in a V-bottom plate.

- The in-filter plate assay procedure is recommended due to its good sample to sample consistency, assay robustness and ease of handling. This procedure requires a vacuum filtration unit for washing (see **Materials to be Provided by the End-User, page 8**). If you have performed bead-based multiplex assays before, your lab may already have the vacuum filtration unit set up.
- If the in-filter plate assay procedure is not possible or if you prefer, the assay can be performed in a V-bottom plate.

### Performing the Assay Using a Filter Plate

- Allow all reagents to warm to room temperature (20-25°C) before use.
  - Set the filter plate on an inverted plate cover at all times during assay setup and incubation steps, so that the bottom of the plate does not touch any surface. Touching a surface may cause leakage.
  - Keep the plate upright during the entire assay procedure, including the washing steps, to avoid losing beads.
  - The plate should be placed in the dark or wrapped with aluminum foil for all incubation steps.
  - Standards and samples should be run in duplicate and arranged on the plate in a vertical configuration convenient for data acquisition and analysis (as shown in attached PLATE MAP, page 33). Be sure to load standards in the first two columns.
1. Pre-wet the plate by adding 100 µL of 1X Wash Buffer to each well and let it sit for 1 minute at room temperature. To remove the excess volume, place the plate on the vacuum manifold and apply vacuum. Do not exceed 10" Hg of vacuum. Vacuum until wells are drained (5-10 seconds). Blot excess Wash Buffer from the bottom of the plate by pressing the plate on a stack of clean paper towels. Place the plate on top of the inverted plate cover.

#### **For measuring cell culture supernatant samples:**

- Add 25 µL of Assay Buffer to all wells.
- Add 25 µL of each standard to the standard wells.
- Add 25 µL of each sample to the sample wells (See **Sample Dilution**)

#### **For measuring serum or plasma samples:**

## Human Anti-Virus Response Panel Mix and Match Subpanel

- Add 25  $\mu\text{L}$  of Matrix B to the standard wells.
  - Add 25  $\mu\text{L}$  of Assay Buffer to the sample wells.
  - Add 25  $\mu\text{L}$  of each standard to the standard wells.
  - Add 25  $\mu\text{L}$  of each diluted serum or plasma sample to the sample wells (See **Sample Dilution**).
2. Vortex mixed beads for 30 seconds. Add 25  $\mu\text{L}$  of mixed beads to each well. The volume should be 75  $\mu\text{L}$  in each well after beads addition. (Note: During beads addition, shake mixed beads bottle intermittently to avoid bead settling).
  3. Seal the plate with a plate sealer. **To avoid plate leaking, do not apply positive pressure to the sealer when sealing the plate.** Wrap the entire plate, including the inverted plate cover, with aluminum foil. Place the plate on a plate shaker, secure it and shake at approximate 500 rpm for 2 hours at room temperature.
  4. **Do not invert the plate!** Place the plate on the vacuum manifold and apply vacuum as before in Step 1. Add 200  $\mu\text{L}$  of 1X Wash Buffer to each well. Remove Wash Buffer by vacuum filtration. Blot excess Wash Buffer from the bottom of the plate with an absorbent pad or paper towels. Repeat this washing step once more.
  5. Add 25  $\mu\text{L}$  of Detection Antibodies to each well.
  6. Seal the plate with a new plate sealer. Wrap the entire plate, including the inverted plate cover, with aluminum foil. Place the plate on a plate shaker and shake at approximately 500 rpm for 1 hour at room temperature.
  7. **Do not vacuum!** Add 25  $\mu\text{L}$  of SA-PE to each well directly.
  8. Seal the plate with a new plate sealer. Wrap the entire plate, including the inverted plate cover, with aluminum foil. Place the plate on a plate shaker and shake at approximate 500 rpm for 30 minutes at room temperature.
  9. Repeat step 4 above.
  10. Add 150  $\mu\text{L}$  of 1X Wash Buffer to each well. Resuspend the beads on a plate shaker for 1 minute.
  11. Read samples on a flow cytometer, preferably within the same day of the assay (Note: Prolonged sample storage can lead to reduced signal).

If the flow cytometer is equipped with an autosampler, read the plate directly using the autosampler. **Please be sure to program the autosampler to resuspend beads in the well immediately before taking samples. The probe height may need to be adjusted when using an autosampler.**




# Human Anti-Virus Response Panel Mix and Match Subpanel

If an autosampler is not available, the samples need to be transferred from the filter plate to FACS tubes and read manually.

## Assay Procedure Summary for Filter Plate


Add 100  $\mu\text{L}$  1X Wash Buffer to filter plate wells  
Vacuum to remove excess buffer




For cell culture supernatant samples,  
Add to the plate:  
25  $\mu\text{L}$  Assay Buffer to all wells  
25  $\mu\text{L}$  diluted standard to standard wells  
25  $\mu\text{L}$  sample to sample wells  
25  $\mu\text{L}$  mixed beads to all wells

For serum and plasma samples,  
Add to the plate:  
25  $\mu\text{L}$  Matrix B to standard wells  
25  $\mu\text{L}$  Assay Buffer to sample wells  
25  $\mu\text{L}$  diluted standard to standard wells  
25  $\mu\text{L}$  sample to sample wells  
25  $\mu\text{L}$  mixed beads to all wells

Incubate 2 hours, RT, shaking



Wash 2 times using vacuum filtration unit  
Add 25  $\mu\text{L}$  Detection Antibodies  
Incubate 1 hr, RT, shaking



 Biotinylated Detection Antibody

Without washing, add 25  $\mu\text{L}$  SA-PE  
Incubate 30 min, RT, shaking

Wash 2 times using vacuum filtration unit  
Add 150  $\mu\text{L}$  of 1x Wash Buffer  
Read on a flow cytometer

## Performing the Assay Using a V-bottom Plate

- Allow all reagents to warm to room temperature (20-25°C) before use.
- Keep the plate upright during the entire assay procedure, including the washing steps, to avoid losing beads.
- The plate should be placed in the dark or wrapped with aluminum foil for all incubation steps.
- Standards and samples should be run in duplicate and arranged on the plate in a vertical configuration convenient for data acquisition and analysis (as shown in attached PLATE MAP, page 33). Be sure to load standards in the first two columns.

### 1. For measuring cell culture supernatant samples:

- Add 25  $\mu$ L of Assay Buffer to all wells.
- Add 25  $\mu$ L of each standard to the standard wells .
- Add 25  $\mu$ L of each sample to the sample wells (See **Sample Dilution**).

### For measuring serum or plasma samples:

- Add 25  $\mu$ L of Matrix B to the standard wells.
  - Add 25  $\mu$ L of Assay Buffer to sample wells.
  - Add 25  $\mu$ L of each standard to standard wells.
  - Add 25  $\mu$ L of each diluted serum or plasma sample to sample wells (See **Sample Dilution**).
2. Vortex mixed beads for 30 seconds. Add 25  $\mu$ L of mixed beads to each well. The volume should be 75  $\mu$ L in each well after beads addition. (Note: During beads addition, shake mixed beads bottle intermittently to avoid bead settling).
  3. Seal the plate with a plate sealer. Cover the entire plate with aluminum foil to protect the plate from light. Shake at 800 rpm on a plate shaker for 2 hours at room temperature (**Depending on the shaker, the speed may need to be adjusted. The optimal speed is one that is high enough to keep beads in suspension during incubation, but not too high so it causes spill from the wells**).
  4. Centrifuge the plate at 1050 rpm (~250 g) for 5 minutes, using a swinging bucket rotor (G.H 3.8) with microplate adaptor (Please refer to **Materials to be Provided by the End-User, page 8**). Do not exceed centrifugation speed as it can affect beads resuspension in later steps.
  5. Immediately after centrifugation, dump the supernatant into the sink by quickly inverting and flicking the plate. Gently blot the plate only once on a stack of clean paper towel. Be careful not to disturb the bead pellet.

## Human Anti-Virus Response Panel Mix and Match Subpanel

Alternatively, removal of the supernatant may be completed using a multichannel pipette set at 75  $\mu\text{L}$ . Try to remove as much liquid as possible without removing any beads. Be sure to change pipette tips between each row or column.


6. **This step is optional.** Wash the plate once by dispensing 200  $\mu\text{L}$  of washing buffer into each well. Shake the plate at 800 rpm for 1 minute and repeat step 4 and 5. Washing may sometimes reduce background, but is not required for this kit.
7. Add 25  $\mu\text{L}$  Detection Antibodies to each well.
8. Seal the plate with a fresh plate sealer. Cover the entire plate with aluminum foil to protect the plate from light. Shake at 800 rpm on a plate shaker for 1 hour at room temperature.
9. **Do not wash the plate!** Add 25  $\mu\text{L}$  of SA-PE to each well directly.
10. Seal the plate with a new plate sealer. Wrap the entire plate with aluminum foil and shake the plate on a plate shaker at approximate 800 rpm for 30 minutes at room temperature.
11. Repeat step 4 and 5.
12. Add 150  $\mu\text{L}$  of 1X Wash Buffer to each well. Resuspend the beads by pipetting.
13. Read samples on a flow cytometer, preferably within the same day of the assay (Note: Prolonged sample storage can lead to reduced signal).

If the flow cytometer is equipped with an autosampler, the samples can be read directly. **Please be sure to program the autosampler to resuspend beads in the well immediately before taking samples. The probe height may need to be adjusted when using an autosampler.**

If an autosampler is not available, the samples can be transferred from the plate to micro FACS (or FACS) tubes and read manually.

# Human Anti-Virus Response Panel Mix and Match Subpanel

## Assay Procedure Summary for V-bottom Plate

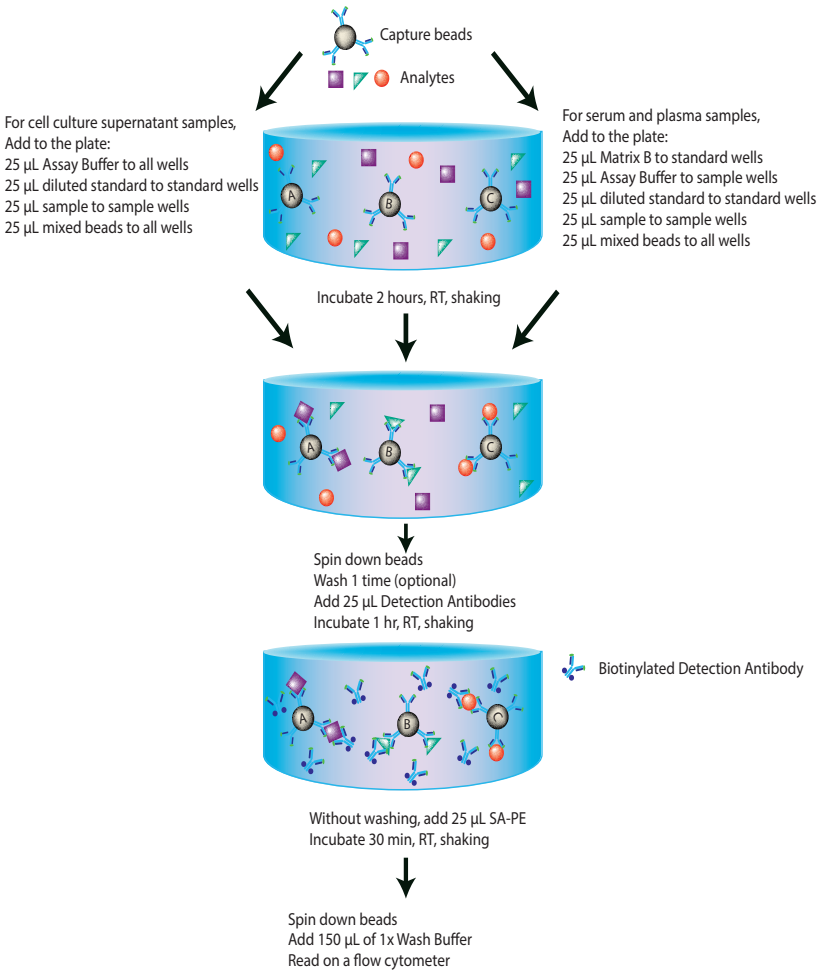

## Chapter 4: FLOW CYTOMETER SETUP

In order to generate reliable data, the flow cytometer must be set up properly before data acquisition.

The setup instructions have been removed from this manual and uploaded onto our website to save paper.

To access the setup instructions, please visit: [www.biolegend.com/legendplex](http://www.biolegend.com/legendplex) and click on the **Instrument Setup** tab.

## Chapter 5: DATA ACQUISITION AND ANALYSIS

### Data Acquisition

1. Before reading samples, make sure that the flow cytometer is set up properly. For flow cytometer setup, please follow the Flow Cytometer Setup guide in this manual or visit: [www.biolegend.com/legendplex](http://www.biolegend.com/legendplex).
2. Create a new template or open an existing template (for details on how to create a cytometer-specific template, please refer to the Flow Cytometer Setup Guide).
3. Vortex each sample for 5 seconds before analysis.
4. Set the flow rate to low. Set the number of beads to be acquired to about 300 per analyte (e.g., acquire 1,500 beads for a 5-plex panel). Do not acquire too many events (e.g. >10,000).

Note: Do not acquire too few or too many beads. Too few beads acquired may result in high CVs and too many beads acquired may result in slow data analysis later.

5. Read samples.

When reading samples, set the flow cytometer to setup mode first and wait until bead population is stabilized before switching to acquisition mode.

To simplify data analysis using the LEGENDplex™ Data Analysis Software, read samples in the same order as shown on the PLATE MAP attached at the end of the manual. For an in-plate assay, read column by column (A1, B1, C1...A2, B2, C2...).

When naming data files, try to use simple names with a consecutive numbering for easy data analysis (e.g. for standards, C0.001, C0.002, C1.003,

## Human Anti-Virus Response Panel Mix and Match Subpanel

C1.004, C2.005, C2.006, C3.007, C3.008, ... C7.015, C7.016; for samples, S1.017, S1.018, S2.019, S2.020, S3.021, S3.022...)

Store all FCS files in the same folder for each assay. If running multiple assays, create a separate folder for each assay.

6. Proceed to data analysis using LEGENDplex™ Data Analysis Software when data acquisition is completed.


### **Data Analysis**

- The assay FCS files should be analyzed using BioLegend's LEGENDplex™ data analysis software. The program is offered free of charge with the purchase of any LEGENDplex™ assay. For further information regarding access to, and use of the program please visit **[biolegend.com/en-us/legendplex](https://www.biolegend.com/en-us/legendplex)**.

## Chapter 6: ASSAY CHARACTERIZATION

### Standard Curve

This standard curve was generated using the LEGENDplex™ Human Anti-Virus Response Panel for demonstration purpose only. A standard curve must be run with each assay.

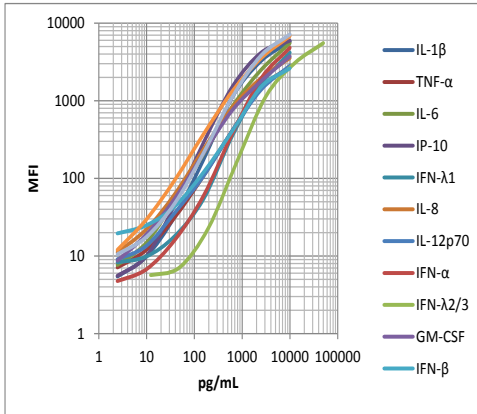

### Assay Sensitivity

The assay sensitivity or minimum detectable concentration (MDC) is the theoretical limit of detection calculated using the LEGENDplex™ Data Analysis Software by applying a 5-parameter curve fitting algorithm.

Analyte	MDC in Cell Culture Medium (pg/mL)	MDC in Serum (pg/mL)
IL-1β	1.3	1.4
IL-6	1.4	1.0
TNF-α	1.1	1.0
IP-10	1.7	2.0
IFN-λ1 (IL-29)	1.7	1.9
IL-8	0.9	1.4
IL-12p70	1.2	1.1
IFN-α2	1.1	1.3
IFN-λ2/3 (IL-28A/B)	7.9	12.8
GM-CSF	1.6	1.1

## Human Anti-Virus Response Panel Mix and Match Subpanel

IFN- $\beta$	1.7	1.5
IL-10	1.1	0.9
IFN- $\gamma$	1.3	0.7

### Cross-Reactivity

The following human recombinant proteins were tested at 50 ng/mL using the LEGENDplex™ Human Anti-Virus Response Panel. There is a 0.4% cross-reactivity between IFN- $\lambda$ 2 protein and the IFN- $\beta$  assay. There is a 95% cross-reactivity between IFN- $\lambda$ 3 protein and the IFN- $\lambda$ 2 Assay. Therefore, the assay detect both IFN- $\lambda$ 2 and IFN- $\lambda$ 3. No or negligible cross-reactivity was found for all other analytes.

IFN- $\lambda$ 1	IFN- $\alpha$ 2	IFN- $\lambda$ 2	IFN- $\beta$	IFN-g	IL-1 $\beta$	IL-6
IL-8	IL-10	IL-12p70	GM-CSF	IP-10	TNF- $\alpha$	IFN- $\alpha$ D
IFN- $\omega$	IL-1 $\alpha$	IL-2	IL-3	IL-4	IL-5	IL-7
IL-9	IL-11	IL-12p40	IL-13	IL-15	IL-17A	IL-17F
IL-17A/F	IL-18	IL-21	IL-22	IL-23	IL-27	IL-33
CCL2	CCL3	CCL4	CCL5	CCL11	CCL17	CCL20
CCL22	CXCL1	CXCL5	CXCL9	CXCL11	sFASL	CCL21
G-CSF	CXCL12	PDGF-BB	TSLP	<b>IFN-<math>\lambda</math>3</b>		

### Accuracy (Spike Recovery)

For spike recovery in cell culture medium, RPMI or DMEM with 10% FCS were spiked with target proteins at three different levels within the assay range. The spiked samples were then assayed, and the measured concentrations were compared with the expected values.

For spike recovery in serum (n=8) and plasma (n=10), samples were first diluted two-fold with Assay Buffer and spiked with target proteins at three different levels within the assay range. The spiked samples were then assayed, and the measured concentrations were compared with the expected values.



## Human Anti-Virus Response Panel Mix and Match Subpanel

Analyte	% of Recovery in RPMI	% of Recovery in DMEM	% of Recovery in Serum	% of Recovery in Plasma
IL-1 $\beta$	99%	95%	79%	84%
IL-6	89%	80%	86%	93%
TNF- $\alpha$	89%	89%	73%	61%
IP-10	96%	93%	64%	83%
IFN- $\lambda$ 1 (IL-29)	117%	112%	137%	135%
IL-8	97%	134%	94%	120%
IL-12p70	94%	74%	70%	80%
IFN- $\alpha$ 2	83%	80%	64%	54%
IFN- $\lambda$ 2/3 (IL-28A/B)	132%	129%	111%	62%
GM-CSF	131%	129%	88%	78%
IFN- $\beta$	92%	99%	84%	104%
IL-10	87%	83%	84%	63%
IFN- $\gamma$	95%	100%	70%	62%

### Linearity of Dilution

For linearity in cell culture medium, 6 cell culture supernatant samples from stimulated PBMCs were serially diluted 1:2, 1:4, 1:8 with Assay Buffer and assayed. The measured concentrations of serially diluted samples were compared with that of the neat samples.

For testing linearity in serum (n=8) and plasma (n=10), samples were first diluted two-fold with Assay Buffer and spiked with a known concentration of target proteins. The spiked samples were serially diluted 1:2, 1:4, 1:8 with Matrix B and assayed. The measured concentrations of serially diluted samples were compared with that of the spiked samples.

Analyte	Linearity in Cell Culture Medium	Linearity in Serum	Linearity in Plasma
IL-1 $\beta$	110%	124%	123%
IL-6	112%	118%	111%
TNF- $\alpha$	106%	141%	137%

## Human Anti-Virus Response Panel Mix and Match Subpanel

IP-10	104%	147%	138%
IFN- $\lambda$ 1 (IL-29)	115%	81%	81%
IL-8	121%	122%	114%
IL-12p70	110%	124%	133%
IFN- $\alpha$ 2	125%	128%	141%
IFN- $\lambda$ 2/3 (IL-28A/B)	97%	114%	121%
GM-CSF	98%	109%	114%
IFN- $\beta$	113%	126%	134%
IL-10	114%	125%	123%
IFN- $\gamma$	112%	126%	132%

### Intra-Assay Precision

Two samples with different concentrations of target proteins were analyzed in one assay with 16 replicates for each sample. The intra-assay precision was calculated as below.

Analyte	Sample	Mean (pg/mL)	STDEV	4%
IL-1 $\beta$	Sample 1	44.99	1.8	4%
	Sample 2	168.19	5.04	3%
IL-6	Sample 1	42.65	2.06	5%
	Sample 2	161.2	10.68	7%
TNF- $\alpha$	Sample 1	45.17	3.93	9%
	Sample 2	149	5.15	3%
IP-10	Sample 1	89.86	2.63	3%
	Sample 2	284.59	10.15	4%
IFN- $\lambda$ 1 (IL-29)	Sample 1	42.39	2.3	5%
	Sample 2	144.41	4.11	3%
IL-8	Sample 1	49.79	2.38	5%
	Sample 2	179.01	11.21	6%
IL-12p70	Sample 1	46.29	2.86	6%
	Sample 2	167.08	9.95	6%
IFN- $\alpha$ 2	Sample 1	42.98	3.96	9%
	Sample 2	159.85	6.29	4%

## Human Anti-Virus Response Panel Mix and Match Subpanel

FN- $\lambda$ 2/3 (IL-28A/B)	Sample 1	39.75	1.49	4%
	Sample 2	126.25	4.76	4%
GM-CSF	Sample 1	44.64	2.98	7%
	Sample 2	168.27	14.4	9%
IFN- $\beta$	Sample 1	39.76	2.62	7%
	Sample 2	147.51	12.46	8%
IL-10	Sample 1	44.41	3.46	8%
	Sample 2	159.91	8.18	5%
IFN- $\gamma$	Sample 1	51.13	2.85	6%
	Sample 2	155.25	8.04	5%

### Inter-Assay Precision

Two samples with different concentrations of target proteins were analyzed in three independent assays with three replicates for each sample. The inter-assay precision was calculated as below.

Analyte	Sample	Mean ( $\mu\text{g/mL}$ )	STDEV	%CV
IL-1 $\beta$	Sample 1	46.3	3.6	8%
	Sample 2	171.6	15.5	9%
IL-6	Sample 1	44.7	3.9	9%
	Sample 2	168.3	13.6	8%
TNF- $\alpha$	Sample 1	43.0	1.4	3%
	Sample 2	160.1	19.0	12%
IP-10	Sample 1	59.8	6.9	12%
	Sample 2	279.7	20.0	7%
IFN- $\lambda$ 1 (IL-29)	Sample 1	40.5	4.0	10%
	Sample 2	155.8	17.2	11%
IL-8	Sample 1	48.5	2.3	5%
	Sample 2	188.6	19.4	10%
IL-12p70	Sample 1	49.7	1.8	4%
	Sample 2	177.5	28.3	16%
IFN- $\alpha$ 2	Sample 1	43.5	2.6	6%
	Sample 2	176.2	16.1	9%

## Human Anti-Virus Response Panel Mix and Match Subpanel

FN- $\lambda$ 2/3 (IL-28A/B)	Sample 1	36.9	2.4	6%
	Sample 2	138.5	23.5	17%
GM-CSF	Sample 1	52.5	7.4	14%
	Sample 2	196.4	33.6	17%
IFN- $\beta$	Sample 1	41.9	4.0	9%
	Sample 2	150.0	7.5	5%
IL-10	Sample 1	50.5	1.5	3%
	Sample 2	168.5	17.0	10%
IFN- $\gamma$	Sample 1	40.2	6.3	16%
	Sample 2	154.0	7.8	5%

## Biological Samples

### Serum and Plasma

Normal human serum samples (n=18) were tested for endogenous levels of the proteins. The concentrations measured are shown below.

Analyte	Range ( $\mu$ g/ml)	% of Detectable	Mean ( $\mu$ g/mL)
IL-1 $\beta$	ND-18.0	39%	2.2
IL-6	ND-45.4	56%	4.6
TNF- $\alpha$	ND-179.9	83%	15.1
IP-10	13.1-84.5	100%	42.0
IFN- $\lambda$ 1 (IL-29)	ND-22.3	56%	6.5
IL-8	3.3-3550.1	100%	418.3
IL-12p70	ND-3.7	22%	0.4
IFN- $\alpha$ 2	ND-44.7	28%	3.4
IFN- $\lambda$ 2/3 (IL-28A/B)	ND-55.4	44%	8.1
GM-CSF	ND-4.3	33%	0.8
IFN- $\beta$	ND-1241.8	39%	99.0
IL-10	ND-0.7	6%	ND
IFN- $\gamma$	ND-1.5	50%	0.4

ND = Non-detectable

## Human Anti-Virus Response Panel Mix and Match Subpanel

Normal human plasma samples (n=22) were tested for endogenous levels of proteins. The concentrations measured are shown below.

Analyte	Range (pg/mL)	% of Detectable	Mean (pg/mL)
IL-1 $\beta$	ND-3.3	23%	0.6
IL-6	ND-3.5	32%	0.7
TNF- $\alpha$	ND-22.0	64%	3.4
IP-10	15.4-83.6	100%	51.4
IFN- $\lambda$ 1 (IL-29)	ND-7.6	36%	1.8
IL-8	3.0-1639.8	100%	158.2
IL-12p70	ND	0%	0.0
IFN- $\alpha$ 2	ND-5.9	14%	0.4
IFN- $\lambda$ 2/3 (IL-28A/B)	ND-19.5	36%	3.8
GM-CSF	ND	0%	0.0
IFN- $\beta$	ND-34.6	41%	6.8
IL-10	ND-2.4	5%	0.1
IFN- $\gamma$	ND-0.9	9%	0.1

ND = Non-detectable

### Cell Culture Supernatant

Human PBMCs ( $1 \times 10^6$  cells/mL) were cultured under various conditions (Unstimulated; LPS, 100 ng/mL; Poly I:C 50  $\mu$ g/mL; CpG, 5  $\mu$ g/mL; R848, 2  $\mu$ g/mL; IFN- $\gamma$ , 100 ng/mL primed for 2 hours + LPS, 1  $\mu$ g/mL). Supernatants were collected after 24 hours and assayed with the LEGENDplex™ Human Anti-Virus Response Panel. The results (all in pg/mL) are summarized below.

Analyte	Control	LPS	Poly IC	CPG	R848	LPS+ IFN- $\gamma$
IL-1 $\beta$	ND	560.6	60.4	ND	263.3	1799.6
IL-6	3.5	7691.4	554.5	16.4	4674.4	14718.7
TNF- $\alpha$	14.3	44.4	15.2	18.8	155.6	4574.1
IP-10	86.9	459.6	12640.0	8865.9	1834.9	5985.6
IFN- $\lambda$ 1 (IL-29)	2.5	13.7	722.0	83.0	45.8	163.9
IL-8	1180.7	>62461.7	1526.3	655.8	28621.7	62461.7

# Human Anti-Virus Response Panel Mix and Match Subpanel

IL-12p70	ND	2.1	76.8	ND	10.0	137.4
IFN- $\alpha$ 2	0.8	4.9	41.4	89.0	157.7	10.7
IFN- $\lambda$ 2/3 (IL-28A/B)	2.4	5.3	66.1	3.8	6.2	7.0
GM-CSF	ND	13.9	3.6	ND	2.9	10.4
IFN- $\beta$	3.5	6.5	19.8	11.8	19.1	12.0
IL-10	1.4	864.9	9.4	2.7	168.1	174.1
IFN- $\gamma$	ND	21.1	1428.0	5.0	66.8	9706.3

ND = Non-detectable

## TROUBLESHOOTING

Problem	Possible Cause	Solution
Bead population shifting upward or downward during acquisition	The strong PE signal from high concentration samples or standards may spill over to classification Channel (e.g., FL3/FL4/APC) and mess up the bead separation.	Optimize instrument settings using Kit Setup Beads, and make appropriate compensation between channels.
Filter plate will not vacuum or some wells clogged	Vacuum pressure is insufficient or vacuum manifold does not seal properly.	Increase vacuum pressure such that 0.2 mL buffer can be suctioned in 3-5 seconds. Clean the vacuum manifold and make sure no debris on the manifold. Press down the plate on the manifold to make a good seal.
	Samples have insoluble particles or sample is too viscous (e.g., serum and plasma samples)	<p>Centrifuge samples just prior to assay setup and use supernatant. If high lipid content is present, remove lipid layer after centrifugation. Sample may need dilution if too viscous.</p> <p>If some wells are still clogged during washing, try the following:</p> <ol style="list-style-type: none"> <li>1). Add buffer to all the wells, pipette up and down the clogged wells and vacuum again.</li> <li>2). Use a piece of clean wipe, wipe the under side of the clogged wells and vacuum again.</li> <li>3). Take a thin needle (e.g., insulin needle), while holding the plate upward, poke the little hole under each of the clogged wells and vacuum again. Do not poke too hard or too deep as it may damage the filter and cause leaking.</li> </ol>
	Filter plate was used without pre-wet.	Pre-wet plate with wash buffer before running the assay.

## Human Anti-Virus Response Panel Mix and Match Subpanel

Insufficient bead count or slow reading	Beads inappropriately prepared	Sonicate bead vials and vortex just prior to addition. Agitate mixed beads intermittently in reservoir while pipetting this into the plate.
	Samples cause beads aggregation due to particulate matter or viscosity.	Centrifuge samples just prior to assay setup and use supernatant. If high lipid content is present, remove lipid layer after centrifugation. Sample may need dilution if too viscous.
	Beads were lost during washing for in-tube assay	Make sure beads are spun down by visually check the pellet (beads are in light blue or blue color). Be very careful when removing supernatant during washing.
	Probe might be partially clogged.	Sample probe may need to be cleaned, or if needed, probe should be removed and sonicated.
Plate leaked	Vacuum pressure set too high	Adjust vacuum pressure such that 0.2 mL buffer can be suctioned in 3-5 seconds. Do not exceed 10" Hg of vacuum.
	Plate set directly on table or absorbent towels during incubations or reagent additions	Set plate on plate holder or raised edge so bottom of filter is not touching any surface.
	Liquid present on the under side of the plate after vacuum	After washing, press down plate firmly on a stack of clean paper towels to dry the underside of the plate.
	Pipette touching and damaged plate filter during additions.	Pipette to the side of wells.
High Background	Background wells were contaminated	Avoid cross-well contamination by changing tips between pipetting when performing the assay using a multichannel pipette.
	Insufficient washes	The background may be due to non-specific binding of SA-PE. Increase number of washes.
Debris (FSC/SSC) during sample acquisition	Debris or platelet may exist in sample solution.	Centrifuge samples before analyzing samples. Remove platelet as much as possible.



## Human Anti-Virus Response Panel Mix and Match Subpanel

Variation between duplicate samples	Beads aggregation	Sonicate and vortex the Beads prior to use.
	Multichannel pipette may not be calibrated or inconsistent pipetting	Calibrate Pipette. Ensure good pipetting practice. Prime pipette before use may help.
	Plate washing was not uniform	Make sure all reagents are vacuumed out completely in all wash steps.
	Samples may contain particulate matters.	Centrifuge samples just prior to assay setup and use supernatant. If high lipid content is present, remove lipid layer after centrifugation. Sample may need dilution if too viscous.
Low or poor standard curve signal	The standard was incorrectly reconstituted, stored or diluted	Follow the protocol to reconstitute, store and dilute standard. Double check your calculation.
	Wrong or short incubation time	Ensure the time of all incubations was appropriate.
Signals too high, standard curves saturated	PMT value for FL2/PE set too high	Make sure the PMT setting for the reporter channel is appropriate
	Plate incubation time was too long	Use shorter incubation time.
Sample readings are out of range	Samples contain no or below detectable levels of analyte	Make sure the experiment to generate the samples worked. Use proper positive controls.
	Samples concentrations higher than highest standard point.	Dilute samples and analyze again.
	Standard curve was saturated at higher end of curve.	Make sure the PMT setting for the reporter channel is appropriate. Use shorter incubation time if incubation time was too long
Missed beads populations during reading, or distribution is unequal	Sample may cause some beads to aggregate.	Centrifuge samples just prior to assay setup and use supernatant. If high lipid content is present, remove lipid layer after centrifugation. Sample may need dilution if too viscous.
	Beads populations are not mixed properly	Make sure all bead populations are mixed. and in similar numbers.

# Human Anti-Virus Response Panel Mix and Match Subpanel

**PLATE MAP (for in-plate assay)**

	1	2	3	4	5	6	7	8	9	10	11	12
<b>A</b>	<b>C0</b>	<b>C4</b>	Sample1	Sample5	Sample 9	Sample 13	Sample 17	Sample 21	Sample 25	Sample 29	Sample 33	Sample 37
<b>B</b>	<b>C0</b>	<b>C4</b>	Sample1	Sample5	Sample 9	Sample 13	Sample 17	Sample 21	Sample 25	Sample 29	Sample 33	Sample 37
<b>C</b>	<b>C1</b>	<b>C5</b>	Sample2	Sample6	Sample 10	Sample 14	Sample 18	Sample 22	Sample 26	Sample 30	Sample 34	Sample 38
<b>D</b>	<b>C1</b>	<b>C5</b>	Sample2	Sample6	Sample 10	Sample 14	Sample 18	Sample 22	Sample 26	Sample 30	Sample 34	Sample 38
<b>E</b>	<b>C2</b>	<b>C6</b>	Sample3	Sample7	Sample 11	Sample 15	Sample 19	Sample 23	Sample 27	Sample 31	Sample 35	Sample 39
<b>F</b>	<b>C2</b>	<b>C6</b>	Sample3	Sample7	Sample 11	Sample 15	Sample 19	Sample 23	Sample 27	Sample 31	Sample 35	Sample 39
<b>G</b>	<b>C3</b>	<b>C7</b>	Sample4	Sample8	Sample 12	Sample 16	Sample 20	Sample 24	Sample 28	Sample 32	Sample 36	Sample 40
<b>H</b>	<b>C3</b>	<b>C7</b>	Sample4	Sample8	Sample 12	Sample 16	Sample 20	Sample 24	Sample 28	Sample 32	Sample 36	Sample 40



LEGENDplex™ Kits are manufactured by **BioLegend**  
8999 BioLegend Way  
San Diego, CA 92121  
Tel: 1.858.768.5800  
Tel: US & Canada Toll-Free: 1.877.Bio-Legend (1.877.246.5343)  
Fax: 1.877.455.9587  
Email: [info@biolegend.com](mailto:info@biolegend.com)  
[biolegend.com](http://biolegend.com)

For a complete list of world-wide BioLegend offices and distributors,  
please visit our website at: [biolegend.com](http://biolegend.com)